


Powder Flow Analyser: Fließfähigkeitstest

Datum: Montag, 20. Oktober 2014 10:46:45

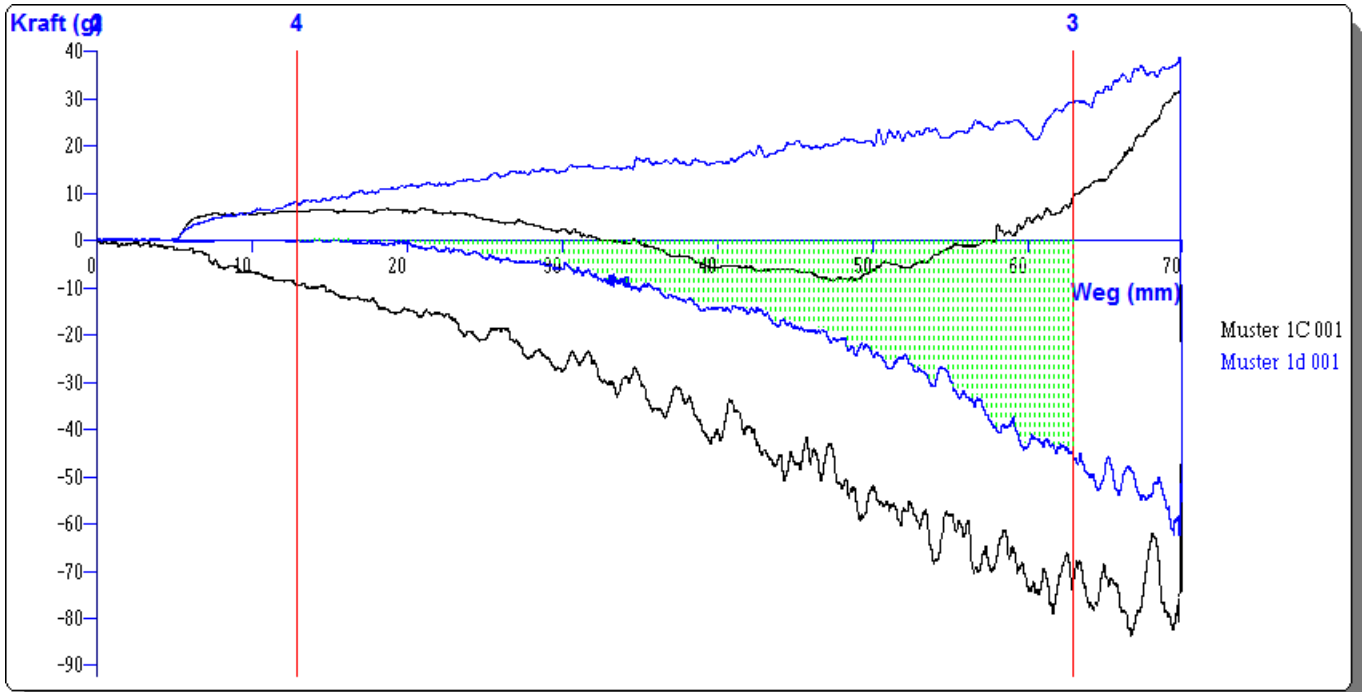

Test ID	Charge	Probengewicht	Fläche (Arbeit) g mm	Fließindex	Schüttdichte g/l
		Variable	Variable	Variable	Variable
Start Charge: Muster 1C	Muster 1C				
Muster 1C 001	Muster 1C	60,352	-1907,452	31,605	431,086
Ende Charge: Muster 1C	Muster 1C				
Start Charge: Muster 1d	Muster 1d				
Muster 1d 001	Muster 1d	75,600	-772,717	10,221	540,003
Ende Charge: Muster 1d	Muster 1d				
Ende Testdaten					

Cohesive Index (CI)	Flow Behaviour
>19	extremely cohesive
19 -16	very cohesive
16 -14	cohesive
14 -11	easy flowing
<11	free flowing